

DRUG

NATIONAL




AUTHORITY

REPORT FOR SAMPLES TESTED FROM JULY- SEPTEMBER (1ST QUARTER) 2017/2018)

DIRECTORATE OF LABORATORY SERVICES
NATIONAL DRUG QUALITY CONTROL LABORATORY

	Medicines	Gloves	Condoms
Received	238	75	11
Tested	110	48	52
Pass	102	36	30
Fail	8	12	22

Samples Tested July – September FY 2017/2018

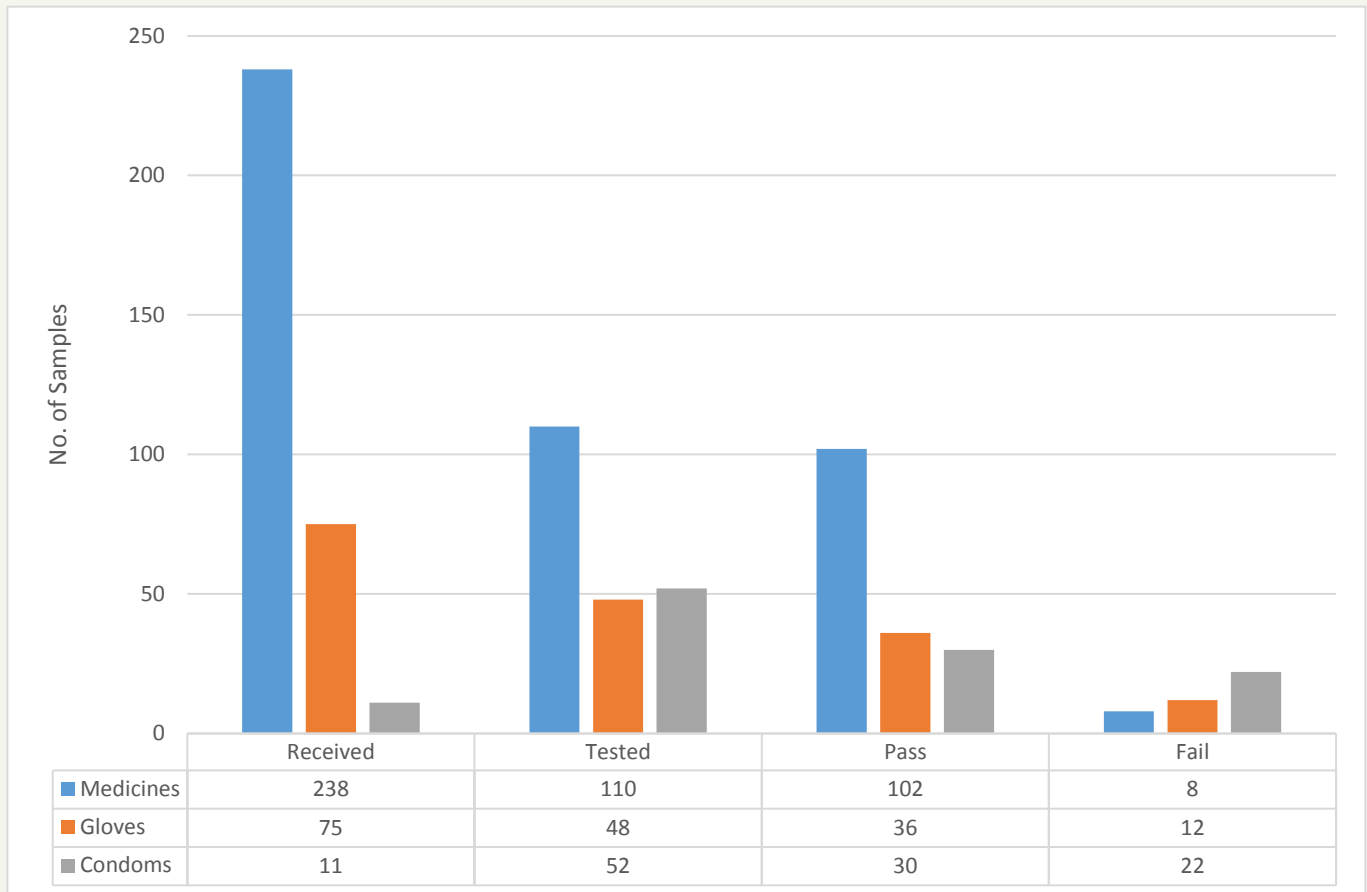

Details of tests failed

1 batch of Lamivudine + Nevirapine + Zidovudine tablets failed labelling requirements

1 batch of Albendazole suspension 2.5% (Veterinary) failed USP specifications for pH

2 batches of Albendazole suspension 10% (Veterinary) failed pH

4 batches of Ciprofloxacin tablets failed dissolution

12 batches of gloves failed holes

14 batches of male condoms failed freedom from holes

5 batches of male condoms failed airburst and holes

3 batches of male condoms failed airburst